

FIG. 1


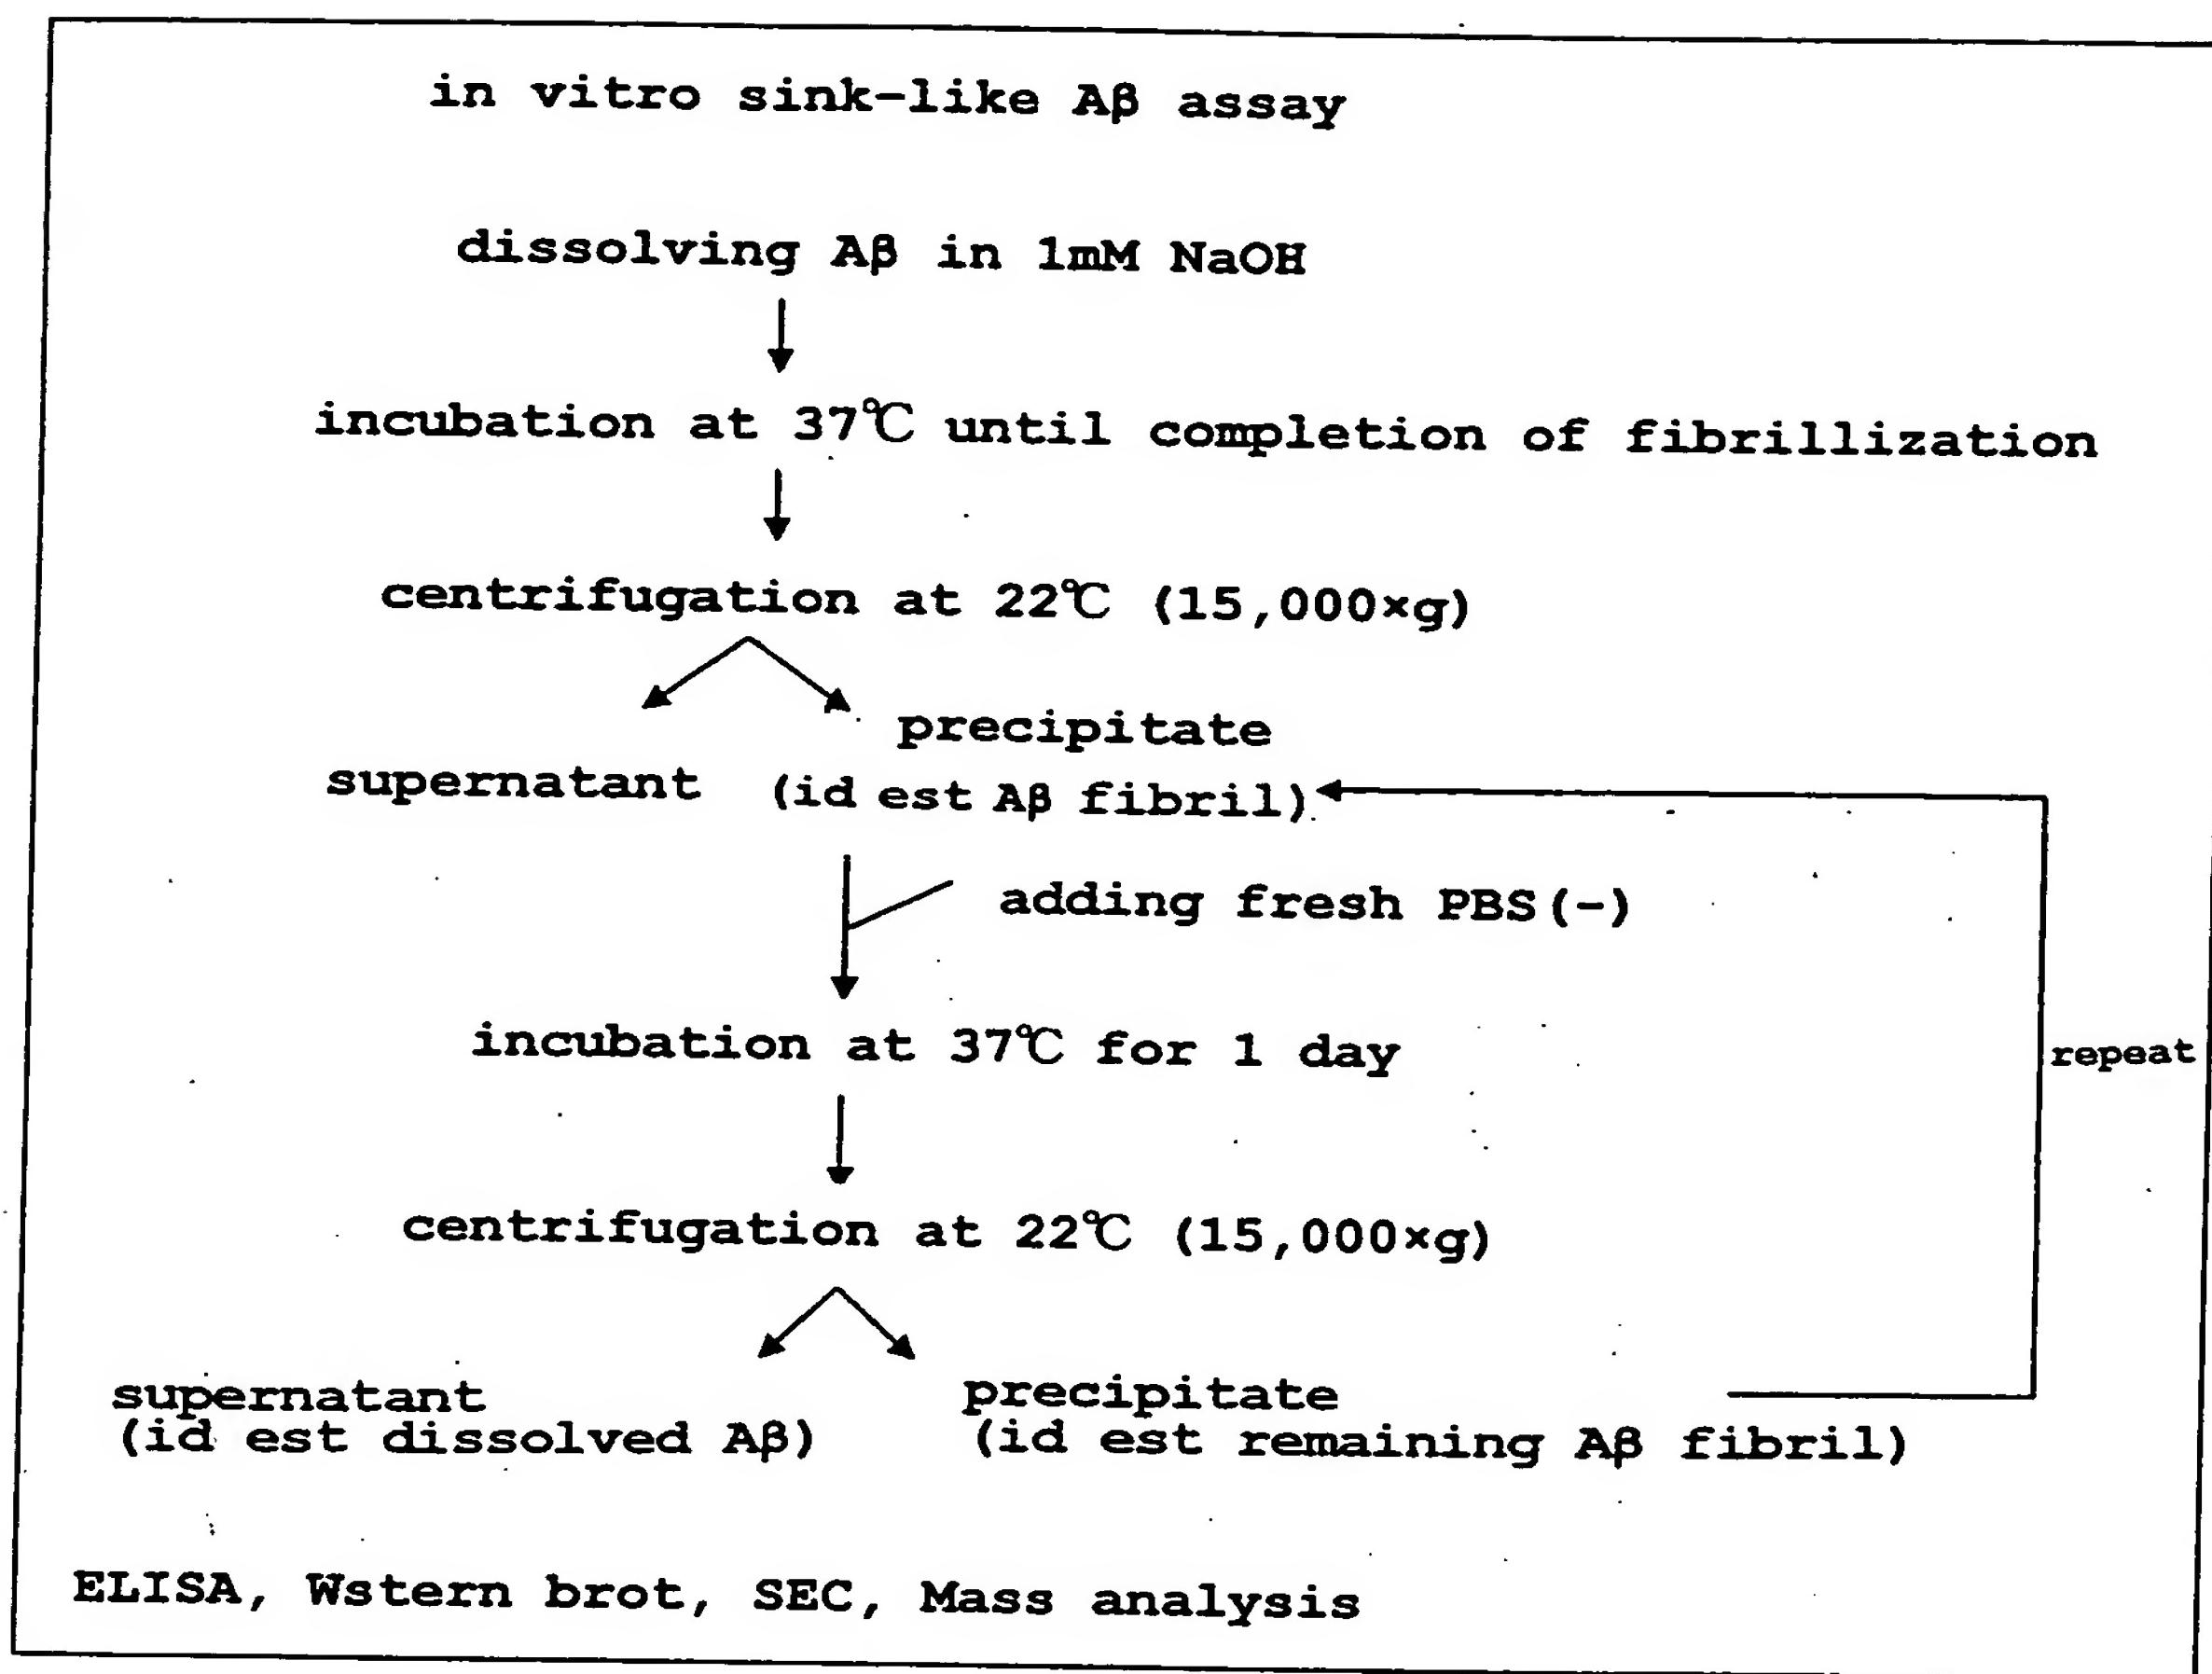



FIG. 2

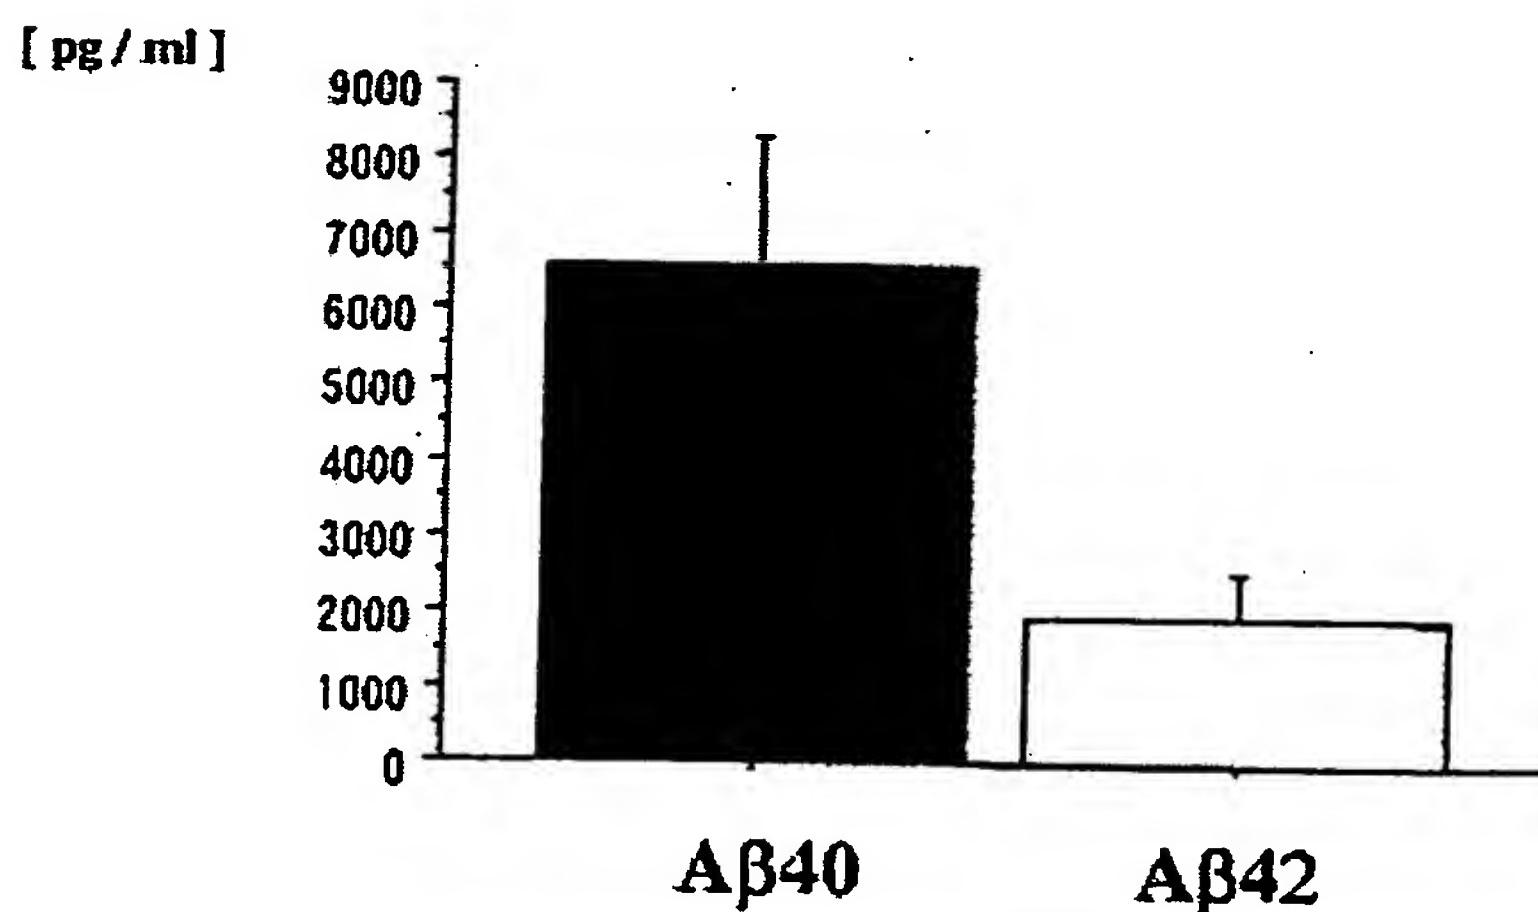


Best Available Copy

FIG. 3

A β 40

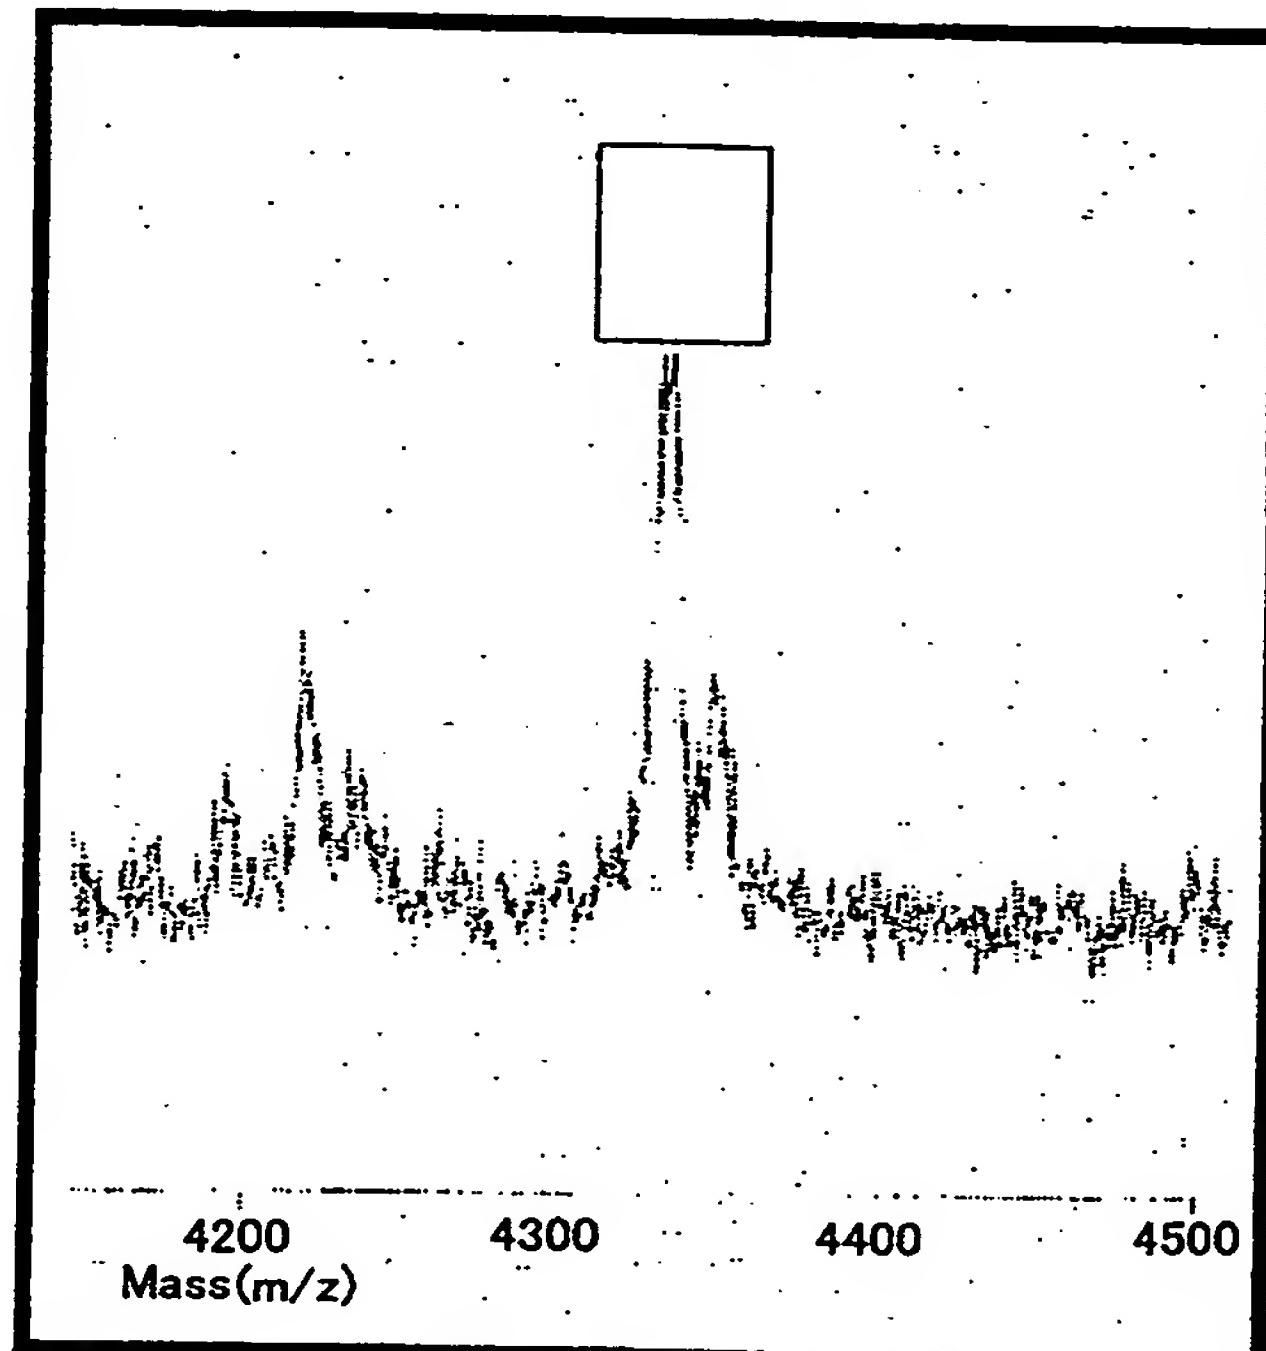

A β 42

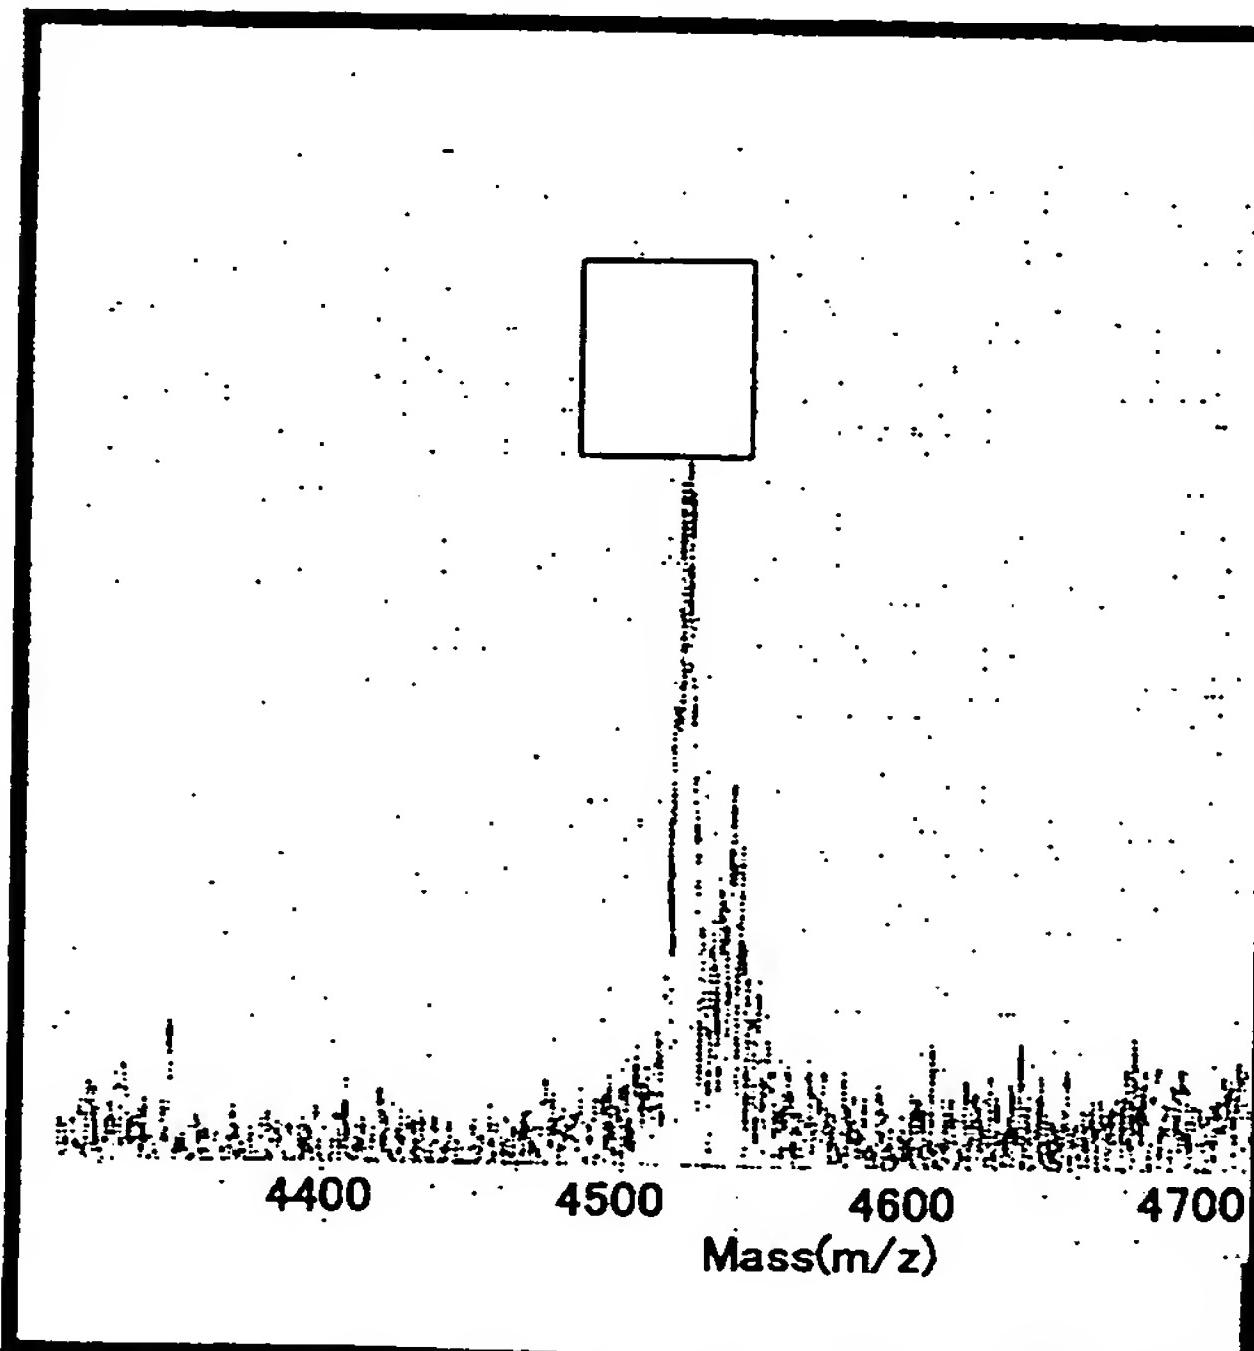

Best Available Copy

FIG. 4

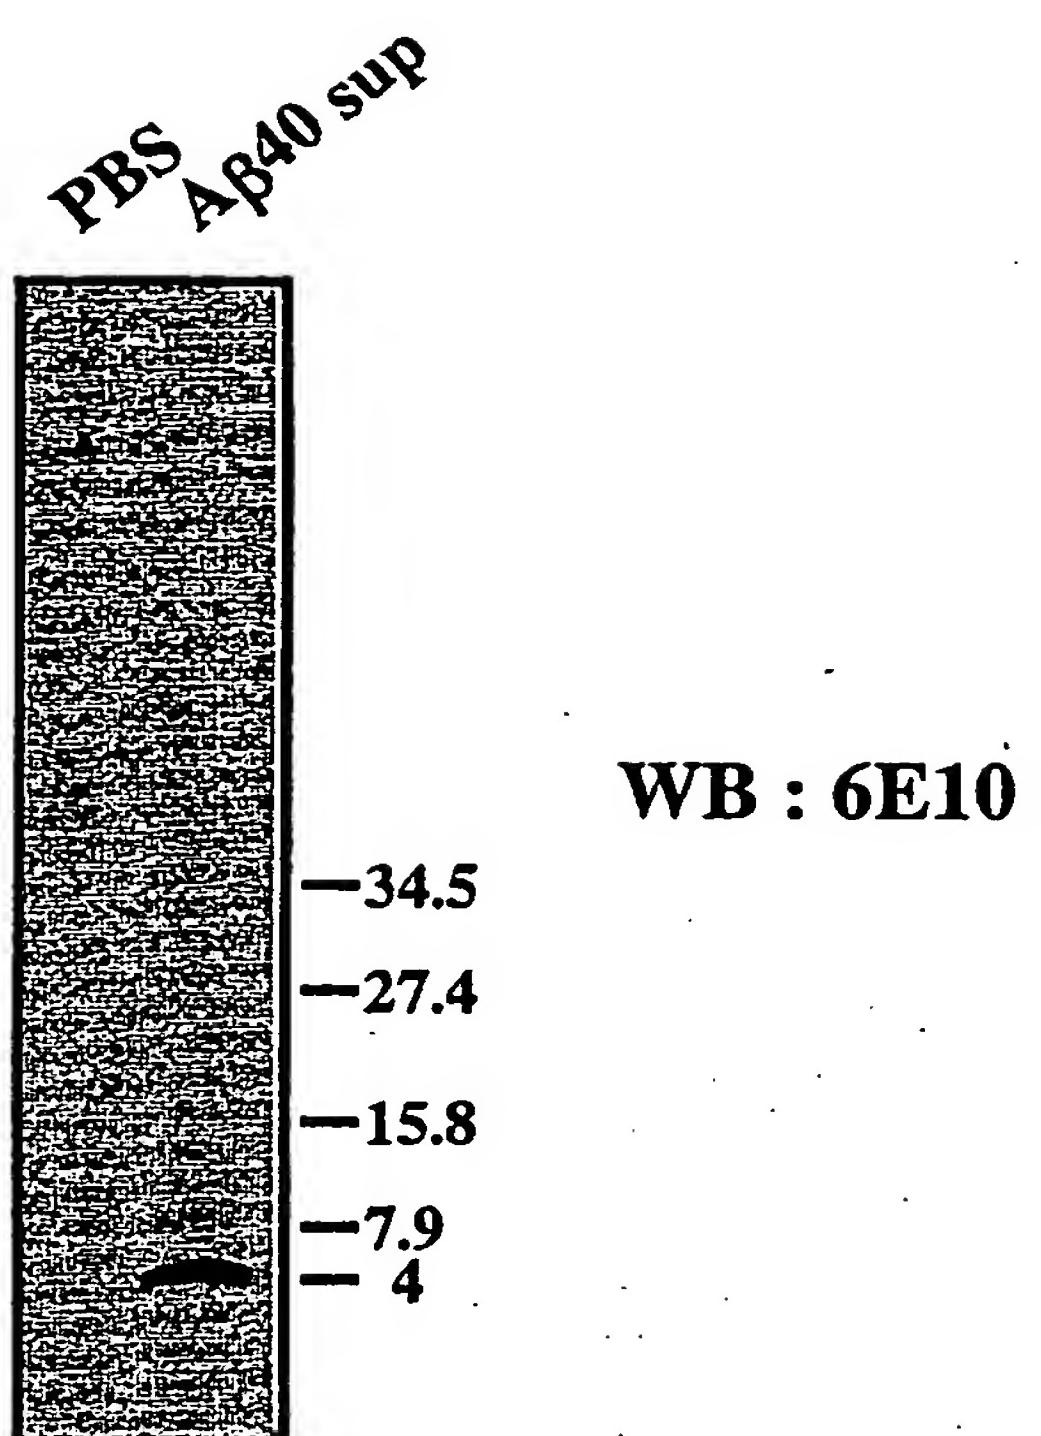


FIG. 5

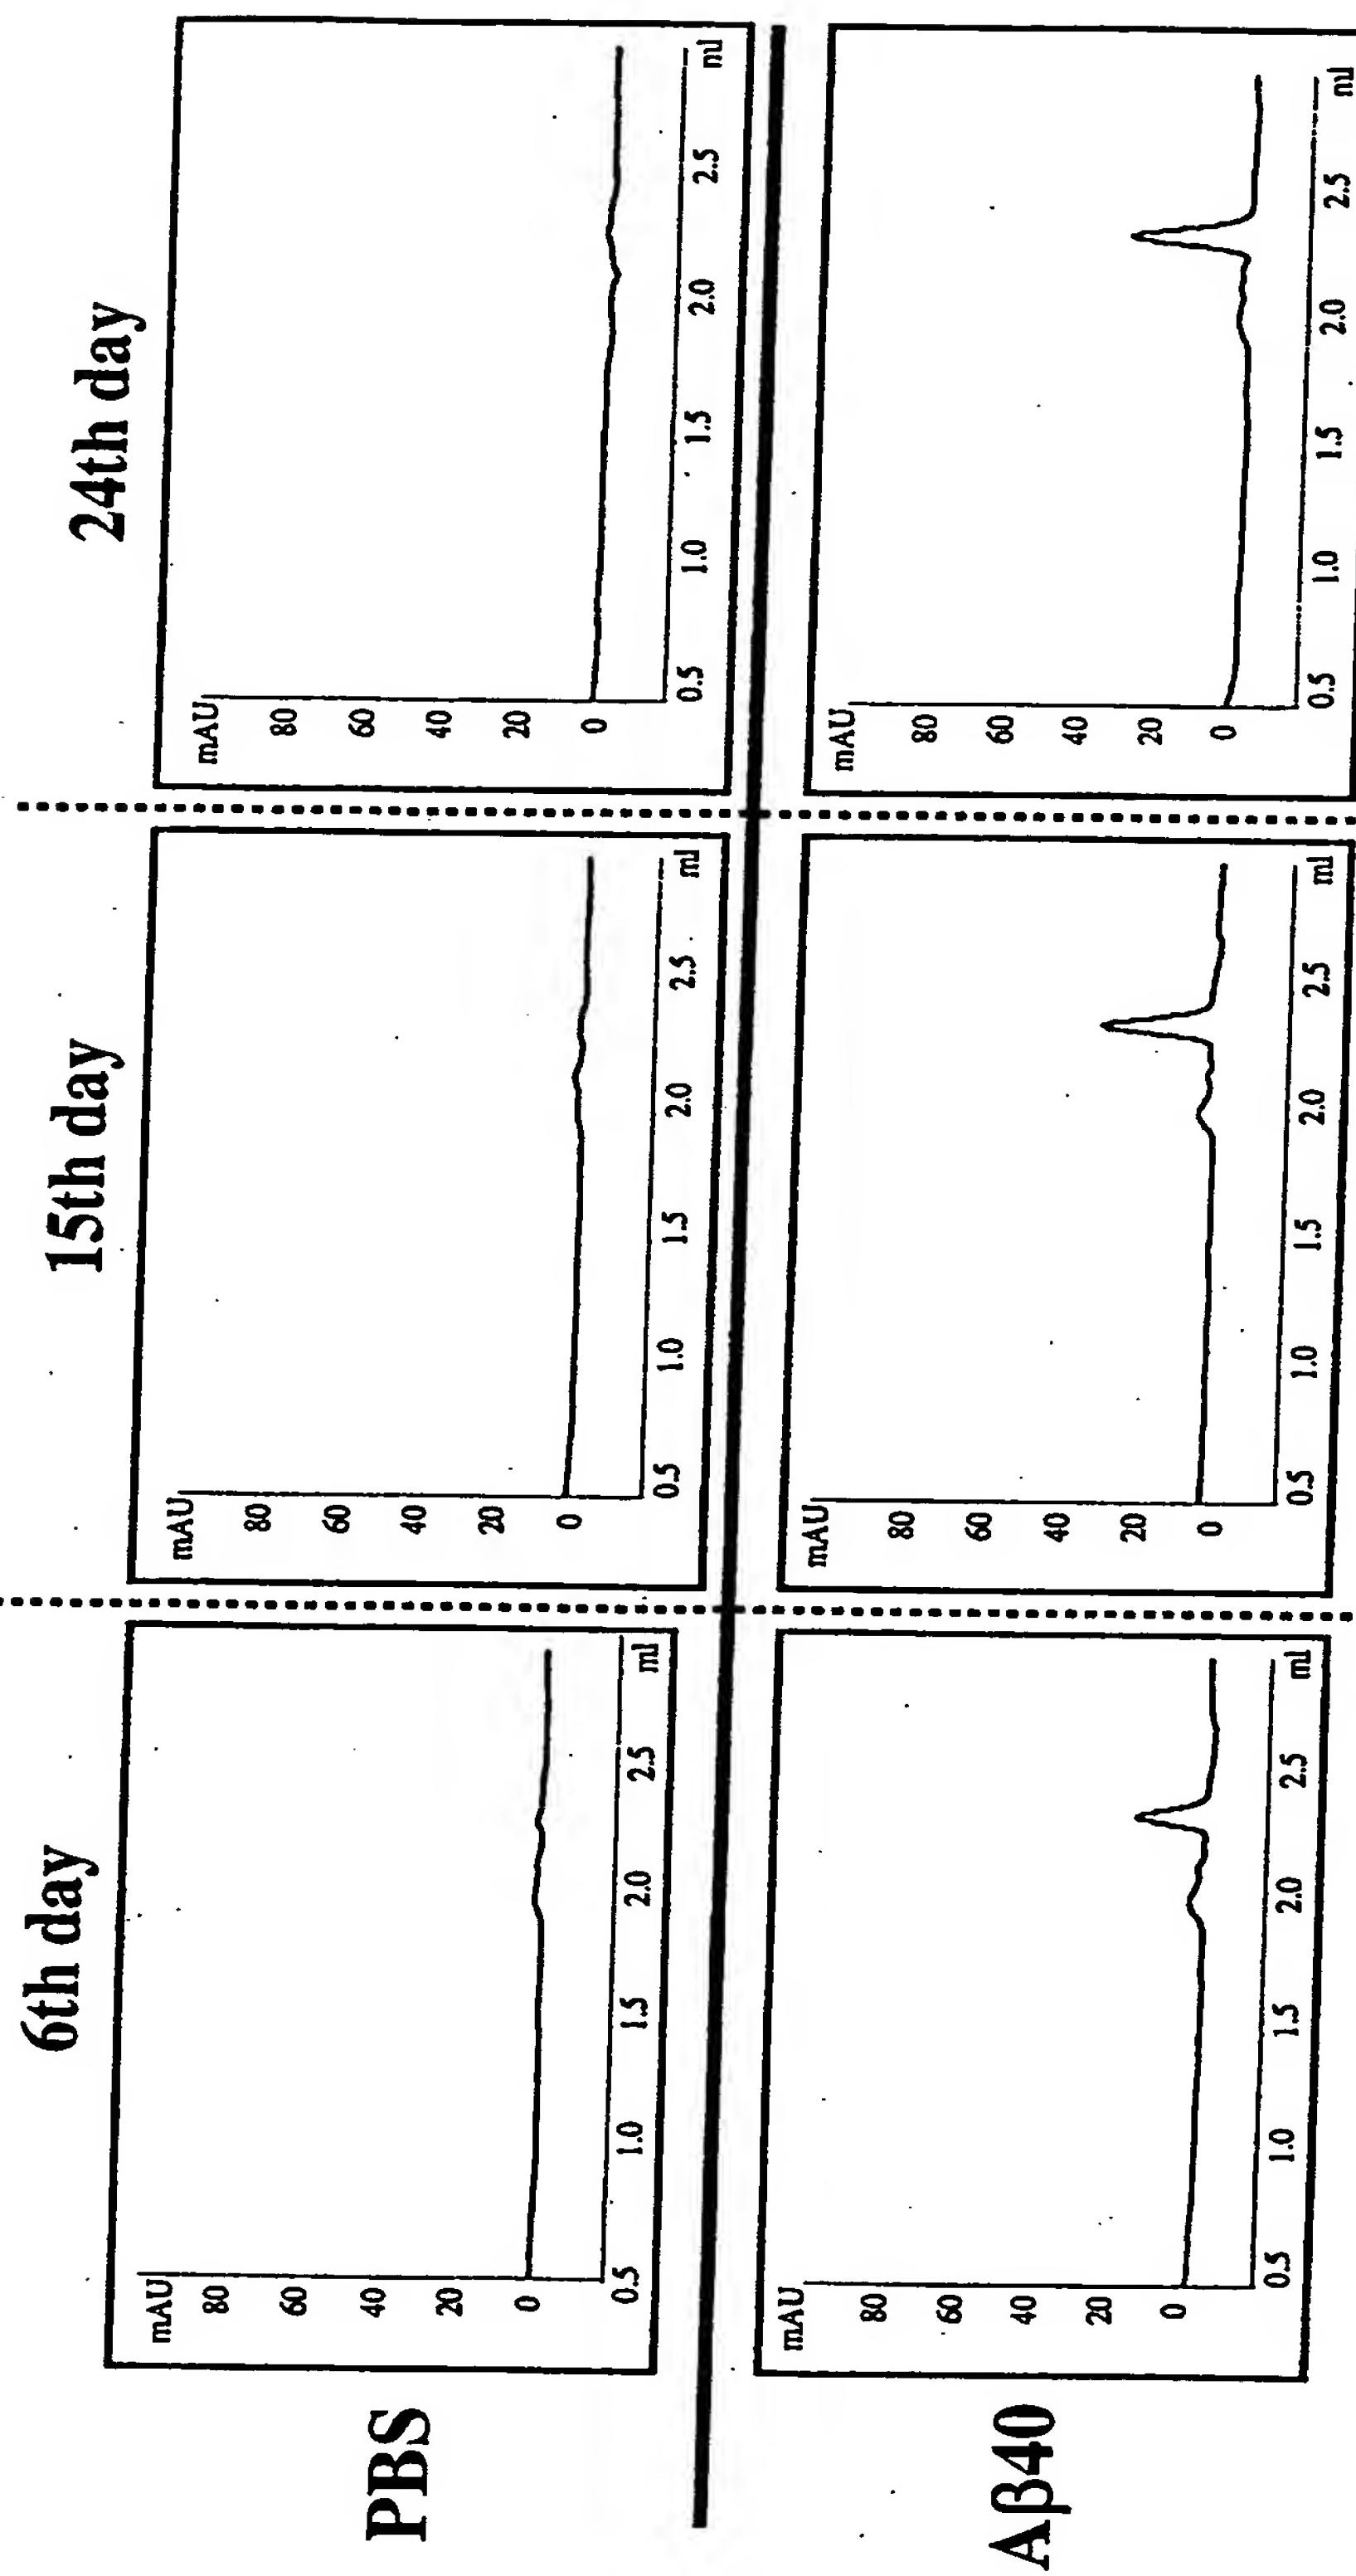


FIG. 6


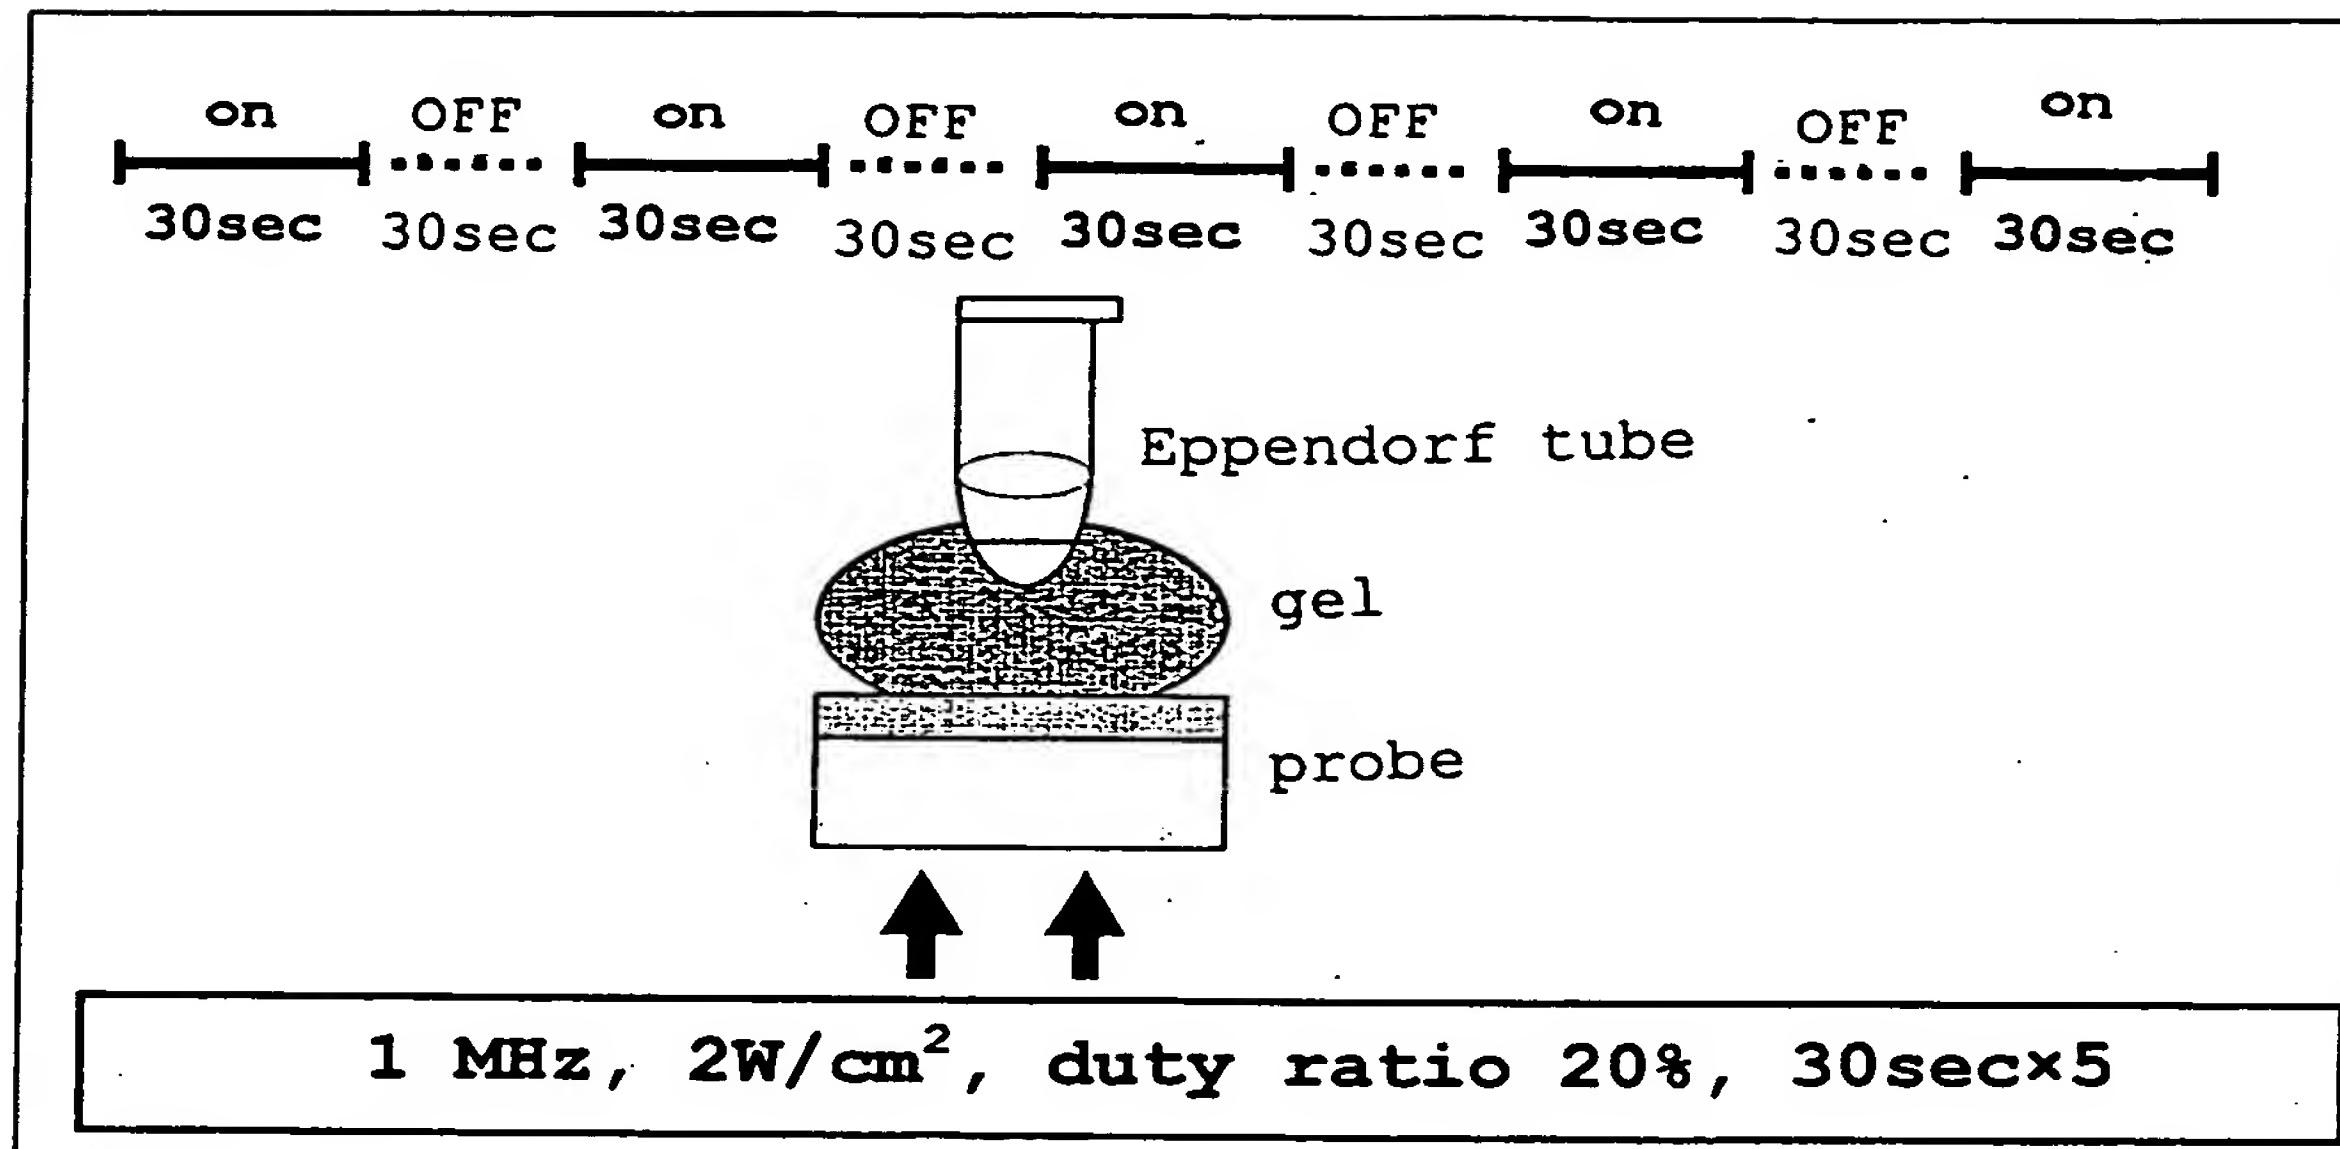


FIG. 7

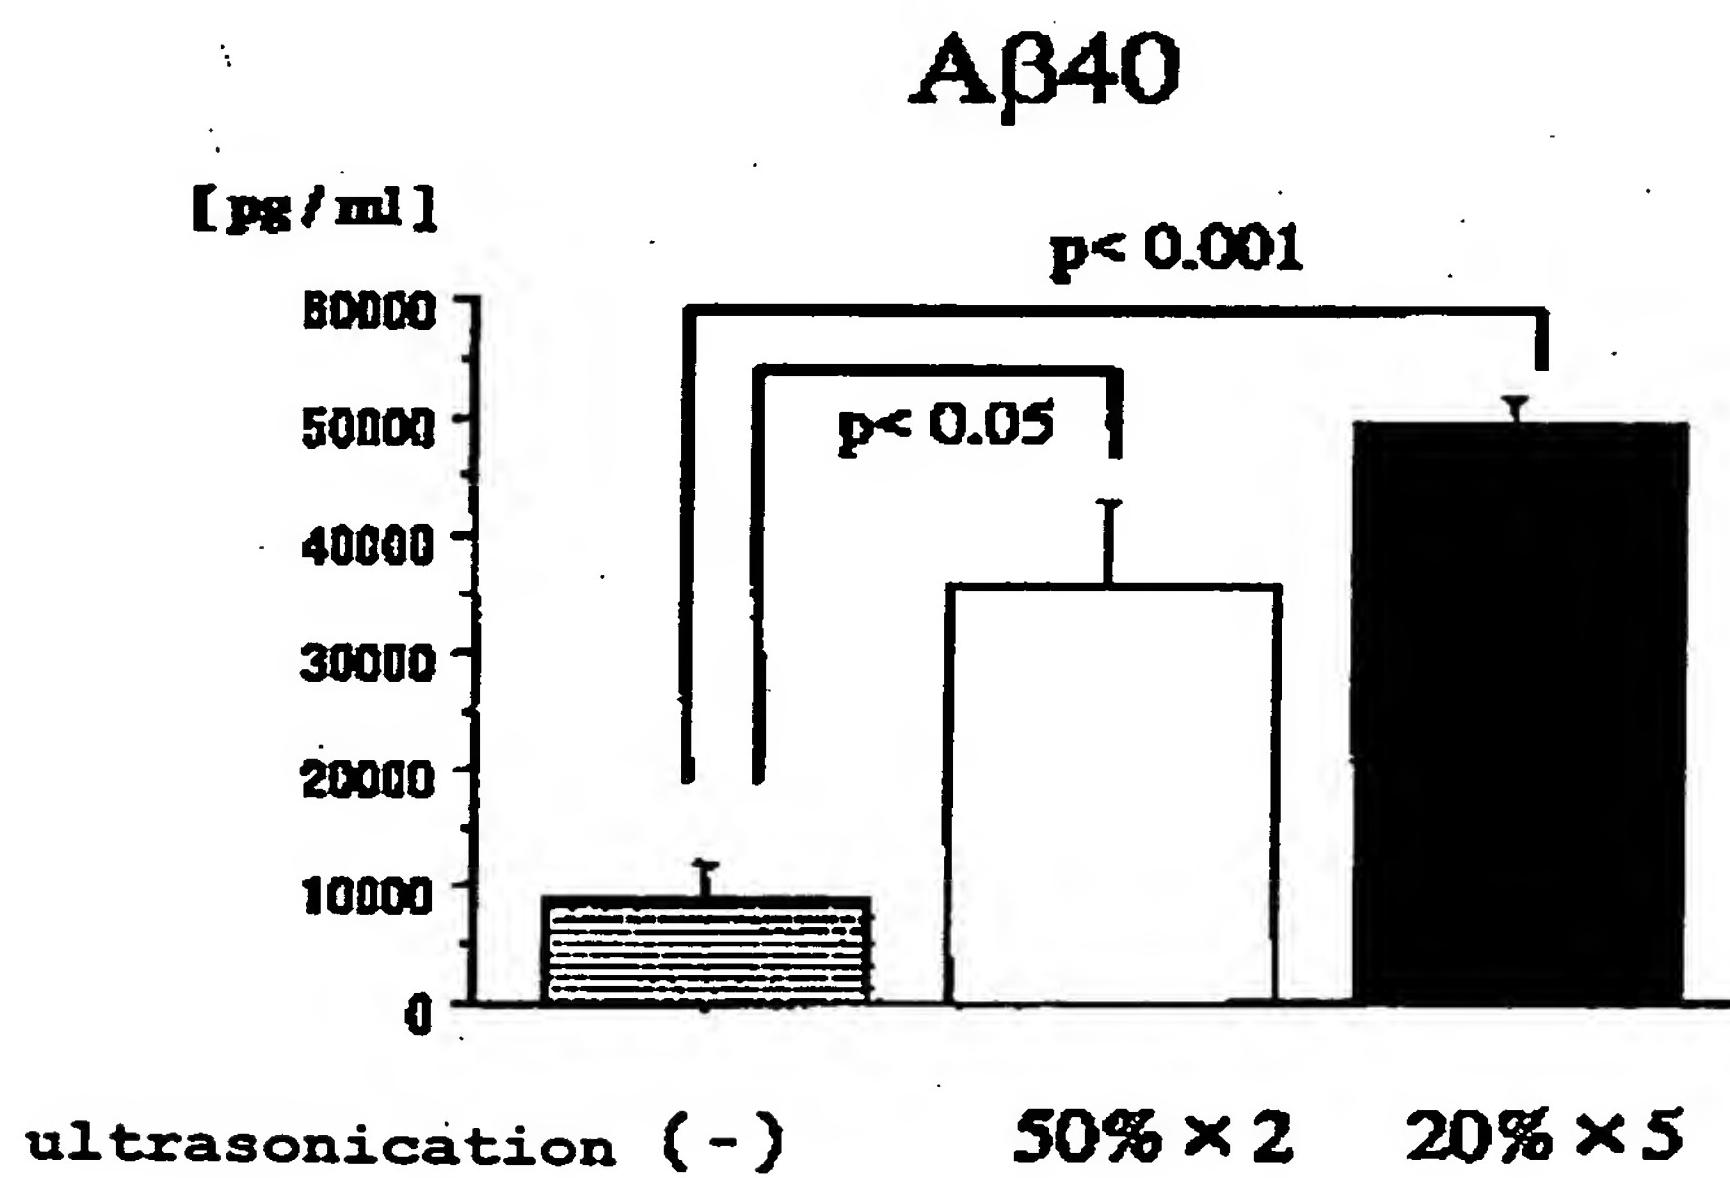

Batch Analytic Chrom

FIG. 8


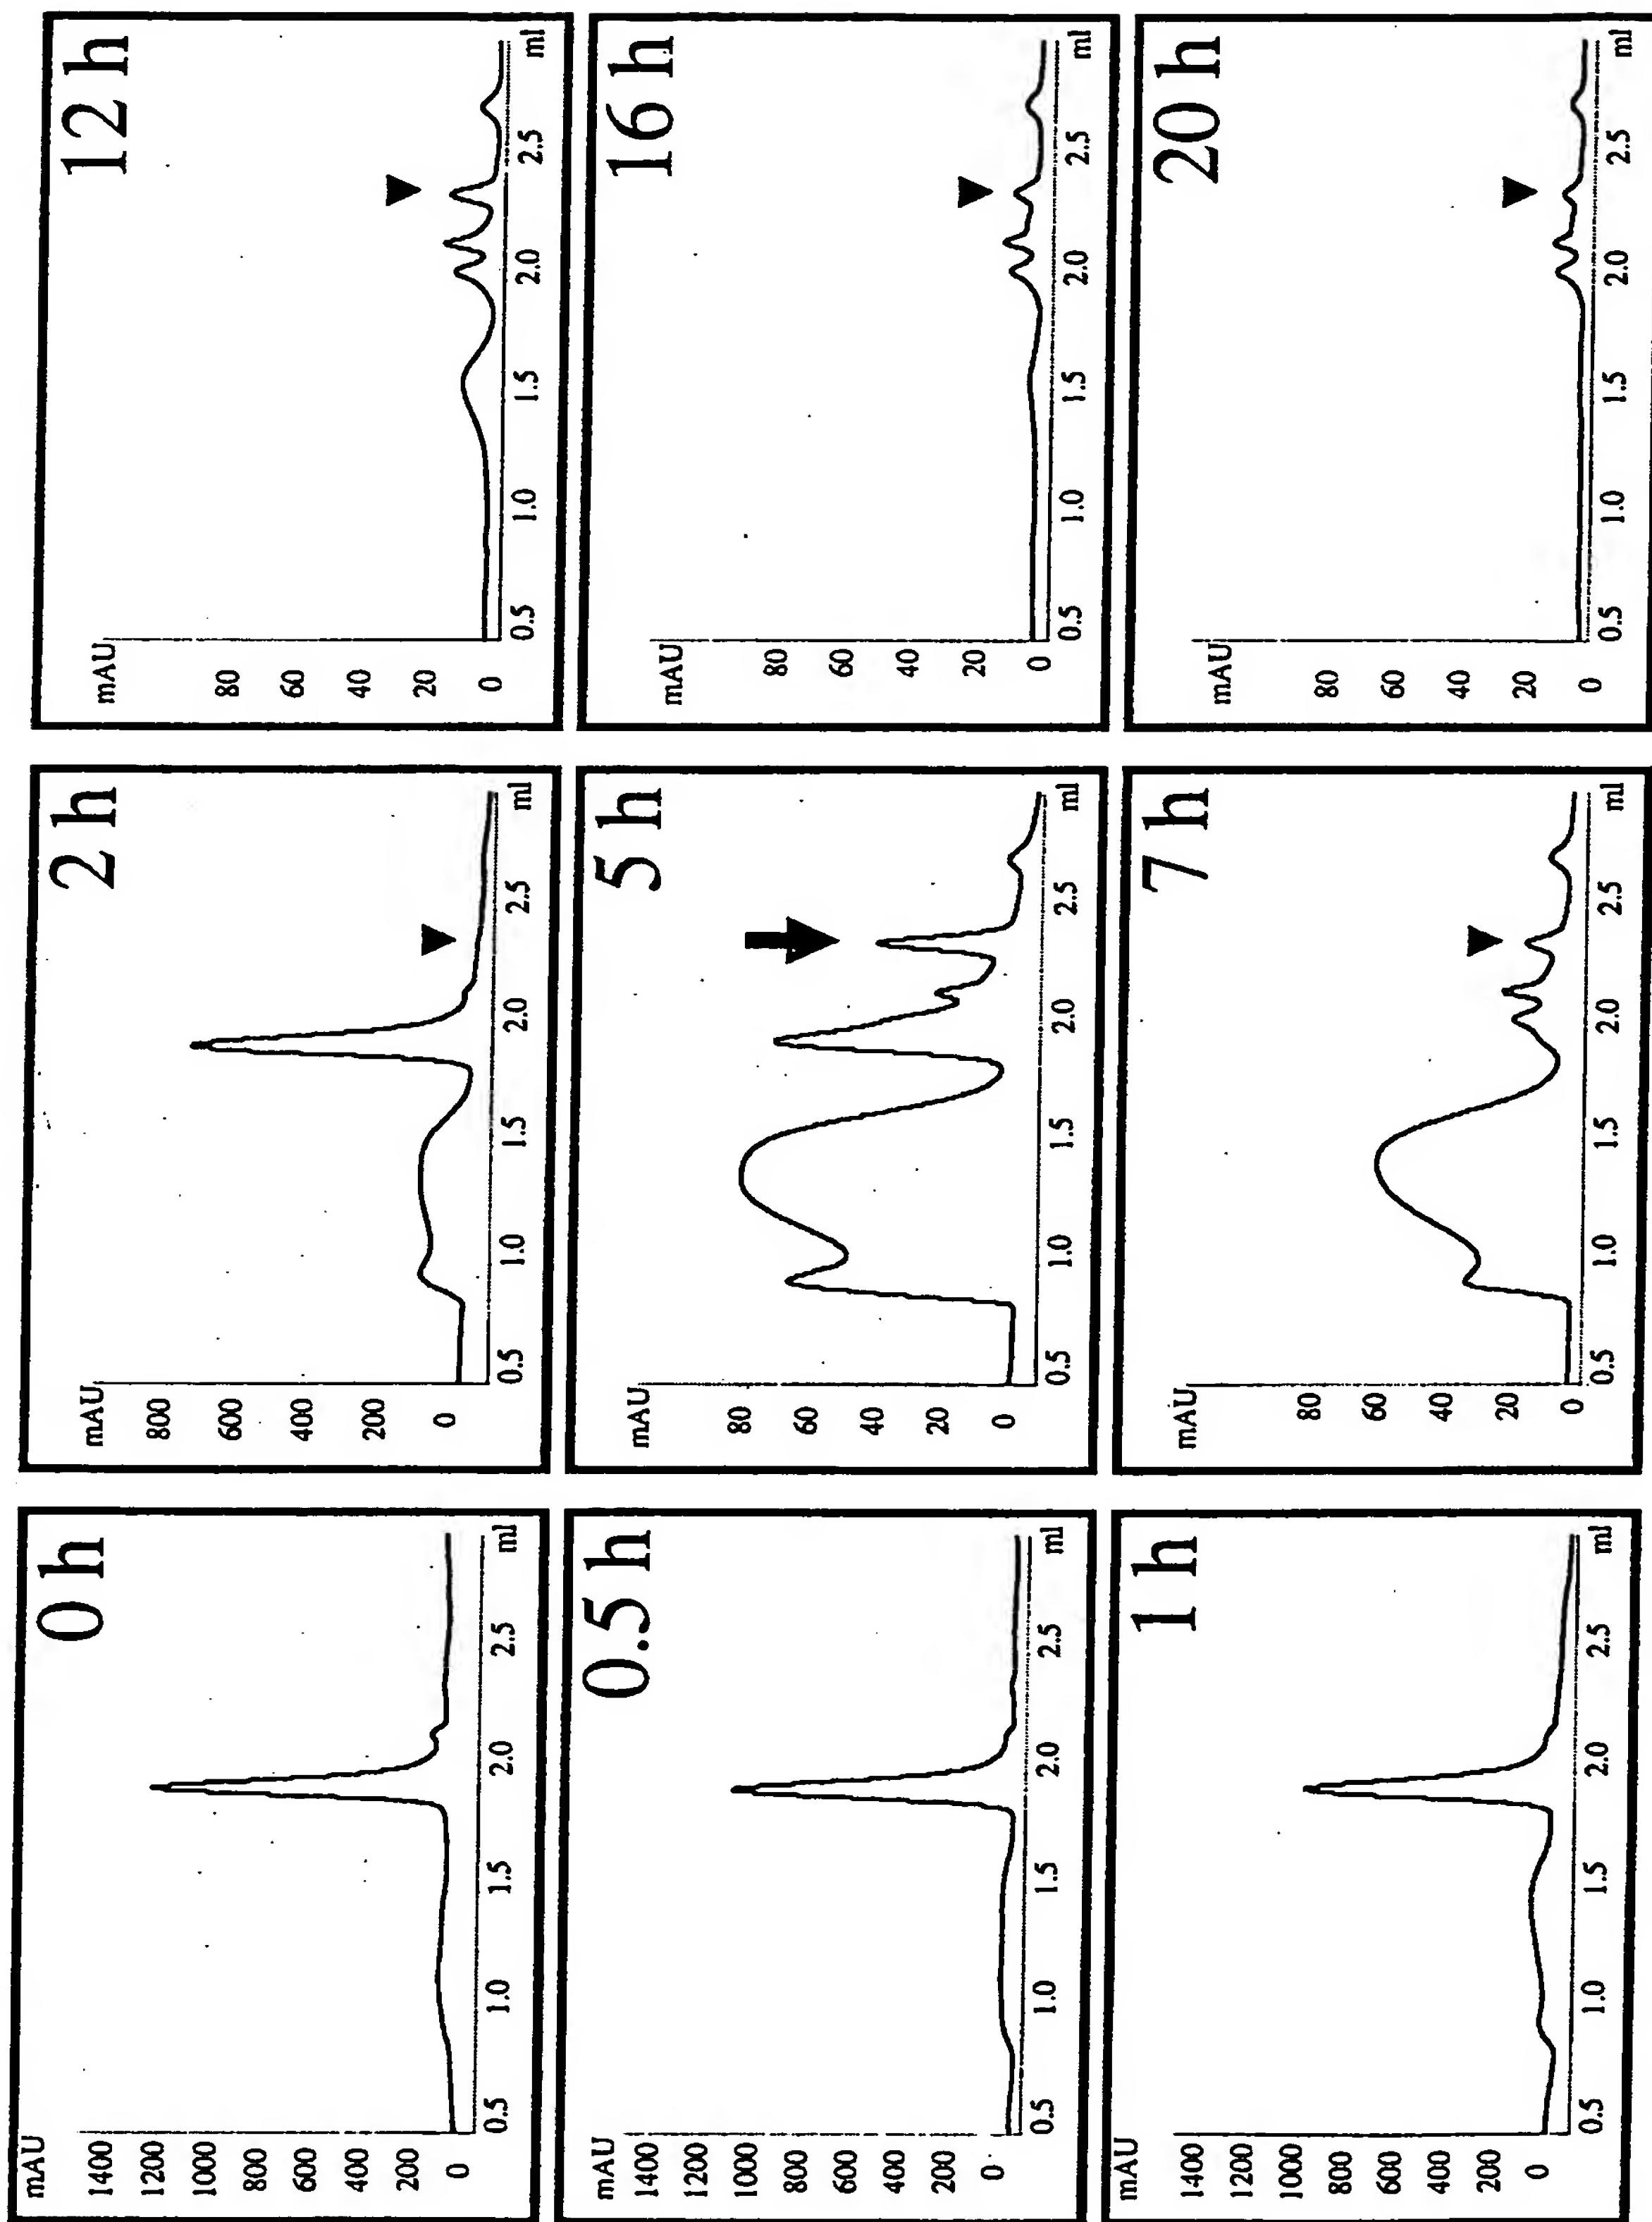


FIG. 9



Best Available Copy

FIG. 10

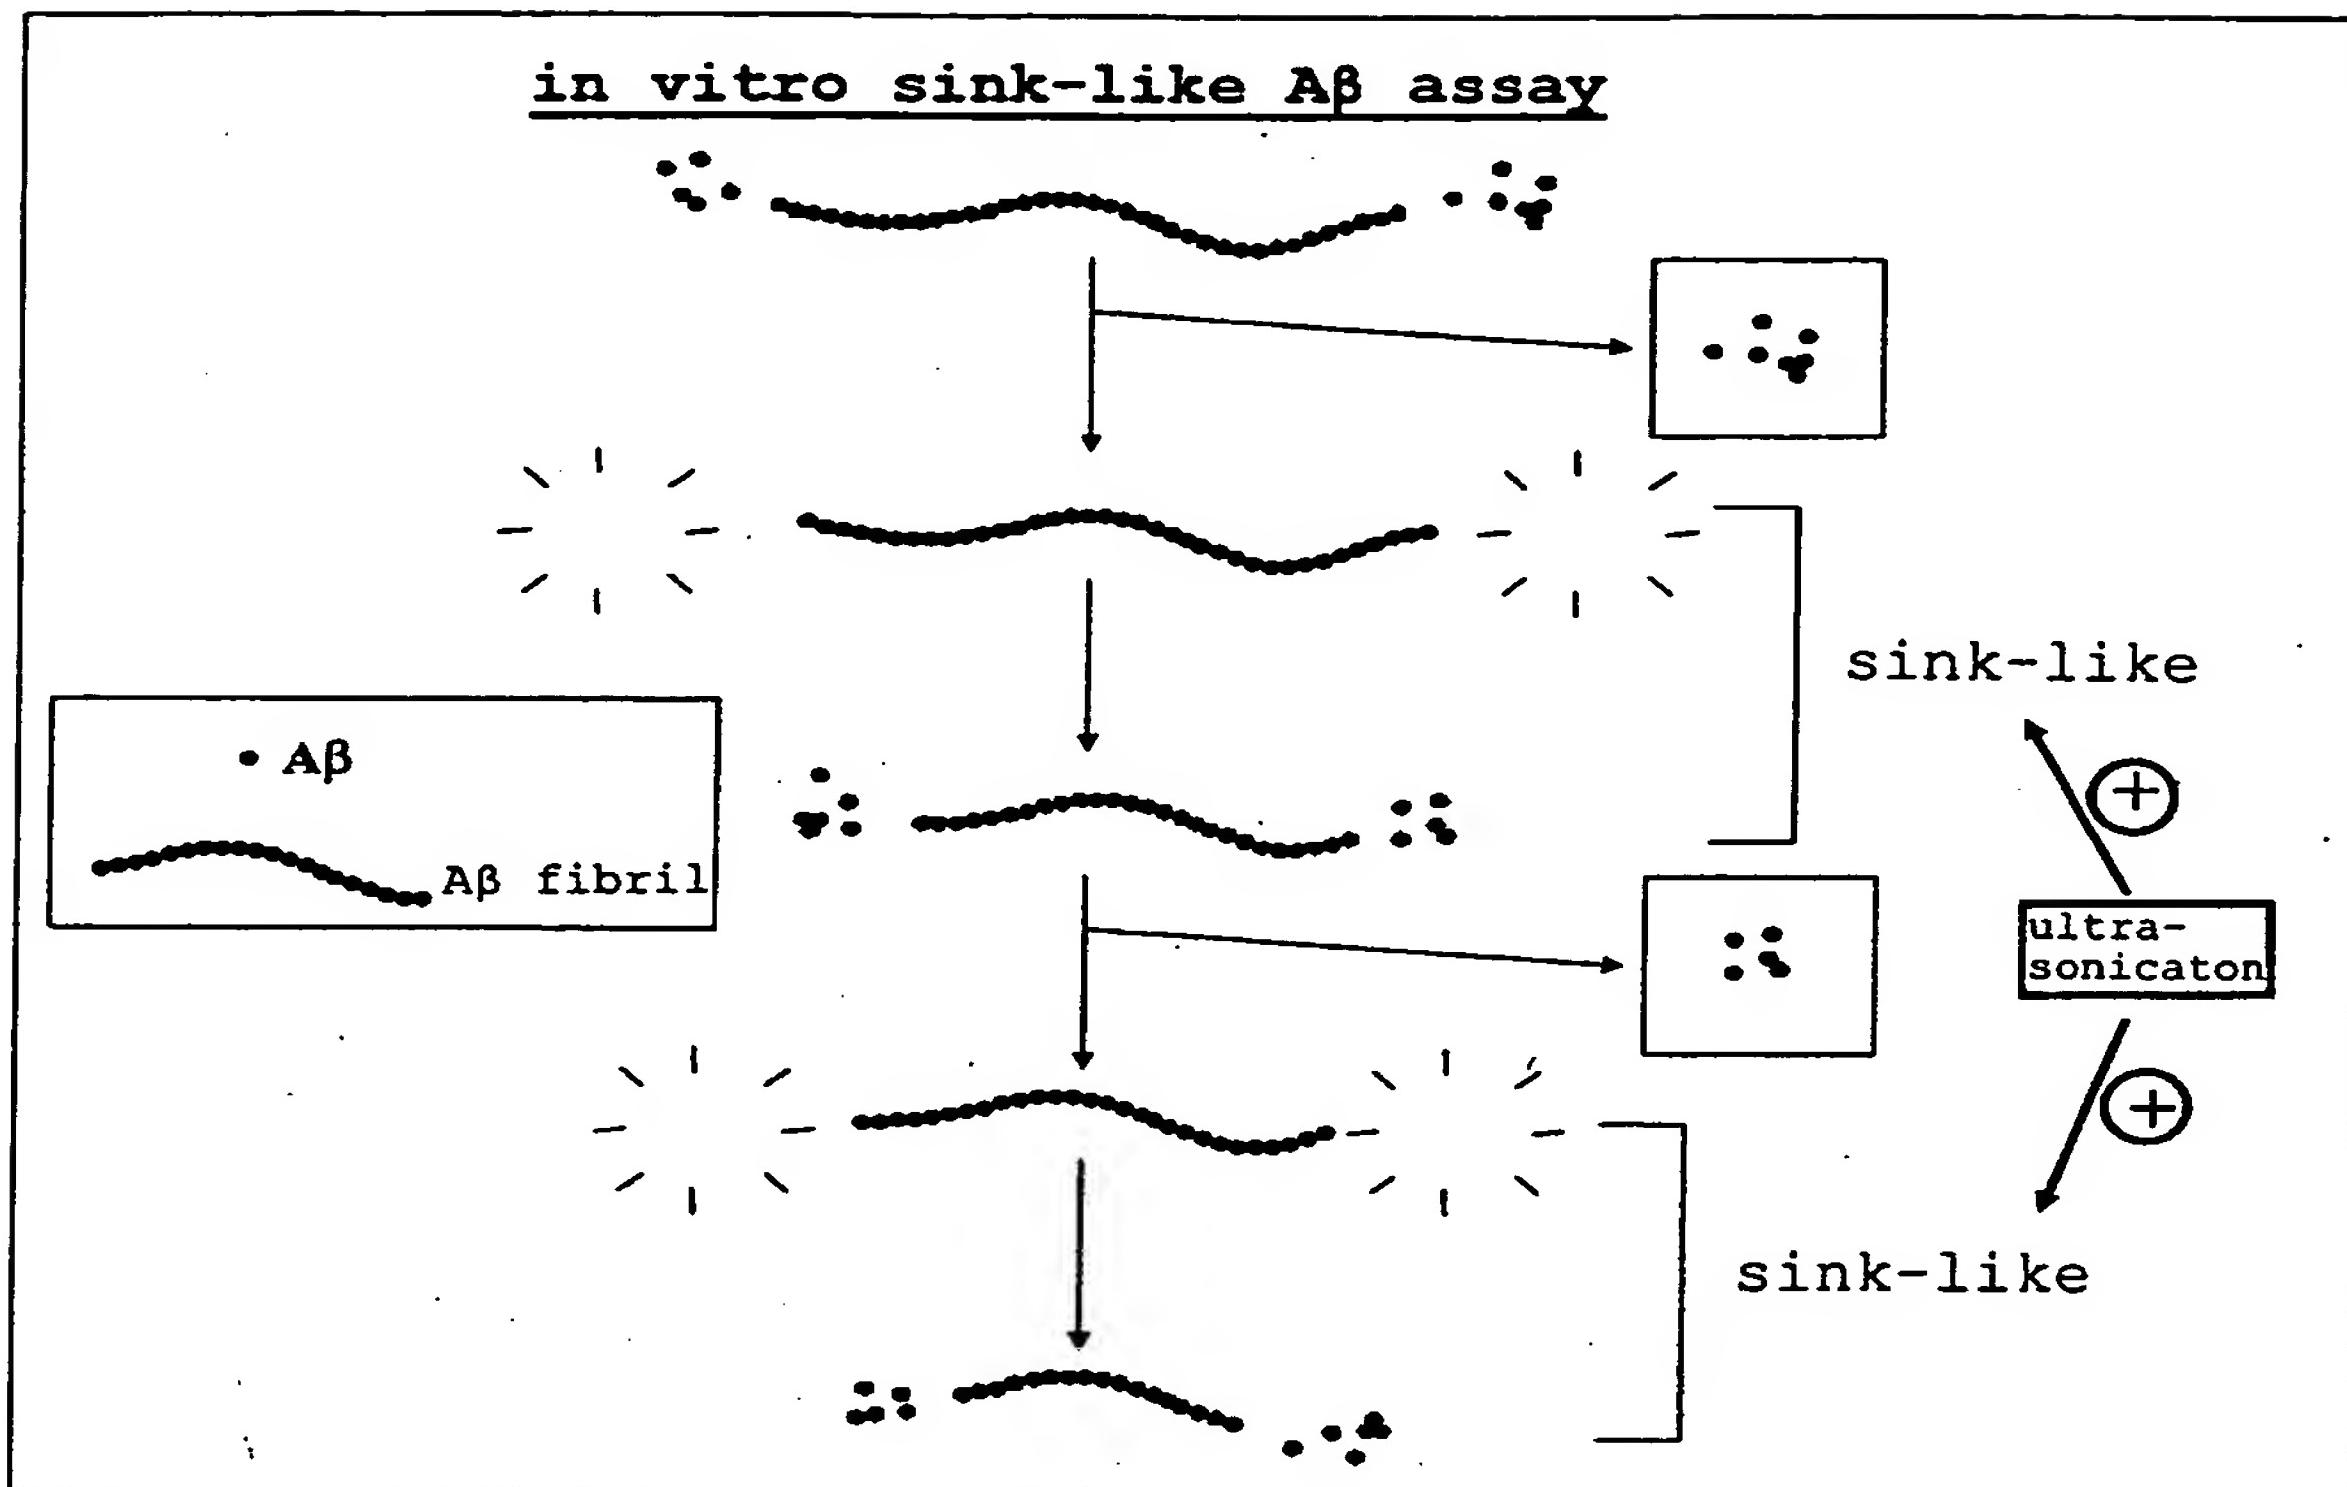